

XPO₂TM
Portable Oxygen
Concentrator

Models XPO100 and XPO100B



DEALER: Keep this manual. The procedures in this manual **MUST** be performed by a qualified technician.

For more information regarding
Invacare products, parts, and services,
please visit www.invacare.com



Yes, you can.

⚠ WARNING

DO NOT USE THIS PRODUCT OR ANY AVAILABLE OPTIONAL EQUIPMENT WITHOUT FIRST COMPLETELY READING AND UNDERSTANDING THESE INSTRUCTIONS AND ANY ADDITIONAL INSTRUCTIONAL MATERIAL SUCH AS OWNER'S MANUALS, SERVICE MANUALS OR INSTRUCTION SHEETS SUPPLIED WITH THIS PRODUCT OR OPTIONAL EQUIPMENT. IF YOU ARE UNABLE TO UNDERSTAND THE WARNINGS, CAUTIONS OR INSTRUCTIONS, CONTACT A HEALTHCARE PROFESSIONAL, DEALER OR TECHNICAL PERSONNEL BEFORE ATTEMPTING TO USE THIS EQUIPMENT - OTHERWISE, INJURY OR DAMAGE MAY OCCUR.

⚠ ACCESSORIES WARNING

INVACARE PRODUCTS ARE SPECIFICALLY DESIGNED AND MANUFACTURED FOR USE IN CONJUNCTION WITH INVACARE ACCESSORIES. ACCESSORIES DESIGNED BY OTHER MANUFACTURERS HAVE NOT BEEN TESTED BY INVACARE AND ARE NOT RECOMMENDED FOR USE WITH INVACARE PRODUCTS.

NOTE: Updated versions of this manual can be found at www.invacare.com.

TABLE OF CONTENTS

SPECIAL NOTES	4
TYPICAL PRODUCT PARAMETERS	5
Regulatory Listing	6
SECTION 1—IMPORTANT SAFEGUARDS	7
Operating Information.....	7
To Reduce The Risk Of Burns, Electrocution, Fire Or Injury To Persons.....	7
Radio Frequency Interference	8
SECTION 2—COMPONENT REPLACEMENT	9
Replacing the Gross Particle Filter or Filter Cover.....	9
Accessing XPO ₂	9
Replacing the Inlet Filter	11
Replacing the Battery.....	12
Re-assembling the XPO ₂	13
Replacement Parts.....	13
SECTION 3—CHECKING O₂ PURITY	14
SECTION 4—ERROR CODES	15
LIMITED WARRANTY	19

SPECIAL NOTES

Signal words are used in this manual and apply to hazards or unsafe practices which could result in personal injury or property damage. Refer to the following table for definitions of the signal words.

SIGNAL WORD	MEANING
DANGER	Danger indicates an imminently hazardous situation which, if not avoided, will result in death or serious injury.
WARNING	Warning indicates a potentially hazardous situation which, if not avoided, could result in death or serious injury.
CAUTION	Caution indicates a potentially hazardous situation which, if not avoided, may result in property damage or minor injury or both.

NOTICE

The information contained in this document is subject to change without notice.

DANGER











DO NOT SMOKE while using this device. Keep all matches, lit cigarettes, candles or other sources of ignition out of the room in which this product is located and away from where oxygen is being delivered.

NO SMOKING signs should be prominently displayed. Textiles and other materials that normally would not burn are easily ignited and burn with great intensity in oxygen enriched air. Failure to observe this warning can result in severe fire, property damage and cause physical injury or death.

CAUTION

“Caution: Federal law restricts this device to sale or rental by or on order of a physician, or any other practitioner licensed by the law of the State in which he/she practices to use or order the use of this device.”

TYPICAL PRODUCT PARAMETERS

	Direct Current
	Type BF equipment
	Attention - Consider Accompanying Documents
	DO NOT smoke
	Class II, Double Insulation
	Power On/Off
	DO NOT dispose of in household waste
	Recycle
	DO NOT use oil or grease
	Keep dry
IPX1	Protected against dripping water

Electrical Requirements:	AC Power Supply: 100-240 VAC 50/60 Hertz
	DC Power Supply: 11-16 VDC
Rated Current Input:	1.0 amps at 120 VAC
	3.3 amps at 18 VDC
Sound Level @ setting 2:	≤ 45dBA weighted
Altitude:	Up to 10,000 ft (3046 m) above sea level
Oxygen Concentration:*	87% to 95.6%, after initial warm-up period (approximately 5 minutes)
*Based on an atmospheric pressure of 14.7 psi (101 kPa) at 70°F (21°C)	
Oxygen Flow:	Pulse flow delivery. Bolus Volume Ranges From 300 - 840cc settings 1 to 5.
Dimensions:	10" high x 7" wide x 4" deep (25.4 cm high x 17.8 cm wide x 10.2 cm deep)
Weight:	6.0 lbs (2.72 kg); 1.3 lbs (0.68 kg) for supplemental battery

TYPICAL PRODUCT PARAMETERS

Battery Duration (times are approximate):	Setting 1 = 3.5 hours
	Setting 2 = 2.5 hours
	Setting 3 = 2.0 hours
	Setting 4 = 1.5 hours
	Setting 5 = 1.0 hours
Battery Recharge Time: <i>NOTE: Recharge time increases if battery is charging while unit is running.</i>	4 hours
Humidity	Operating Humidity: 15% to 60% non condensing
	Storage Humidity: up to 95% non condensing
Temperature Range: (All power sources)	Operating temperature: 41°F to 95°F (5°C to 35°C)
	Storage temperature: -2°F to 140°F (-20°C to 60°C)
Extended Temperature Range: (Using AC or DC adapters)	Operating Temperature: 95°F to 104°F (35°C to 40°C) Continuous use - all settings
Extended Temperature Range (Using Internal Battery)	Operating Temperature: 95°F to 104°F (35°C to 40°C) Continuous use - settings 1, 2 and 3 45 minutes (max) - setting 4 30 minutes (max) - setting 5

Regulatory Listing

ETL certified complying with:	EN 55011:1998
	CISPR 11: 2003
	IEC 60601-1; 2nd ed. 2005
	IEC 60601-1-2; 2.1 ed.
	IEC 61000-3-2:2005
	IEC 61000-3-3:2005
	UL 60601-1, 1st ed.
	CSA 601.1 M90

SECTION I—IMPORTANT SAFEGUARDS

In order to ensure the safe installation, assembly and operation of the XPO₂ Portable Concentrator these instructions **MUST** be followed.

⚠ WARNING

SECTION 1 - IMPORTANT SAFEGUARDS contains important information for the safe operation and use of this product.

Operating Information

⚠ DANGER

A spontaneous and violent ignition may occur if oil, grease, greasy substances, or petroleum based products come in contact with oxygen under pressure. These substances **MUST** be kept away from the XPO₂ portable concentrator, tubing and connections, and all other oxygen equipment. **DO NOT** use any lubricants unless recommended by Invacare.

To Reduce The Risk Of Burns, Electrocution, Fire Or Injury To Persons

DO NOT come in contact with the concentrator while wet.

DO NOT place or store product where it can drop into water or other liquid.

DO NOT reach for product that has fallen into water. Unplug **IMMEDIATELY**.

Avoid creation of any spark near medical oxygen equipment. This includes sparks from static electricity created by any type of friction.

NEVER drop or insert any object or liquid into any opening.

For optimum performance, Invacare recommends that each concentrator be On, in auto-pulse mode, and running for a minimum of 5 minutes. Shorter periods of operation may reduce maximum product life. Refer to Checking O₂ Purity on page 14 for auto-pulse mode.

A product should **NEVER** be left unattended when plugged in. Make sure XPO₂ is Off when not in use.

The XPO₂ **MUST** be used in an upright position.

DO NOT connect the concentrator in parallel or series with other oxygen concentrators or oxygen therapy devices.

Radio Frequency Interference

This equipment has been tested and found to comply with EMC limits specified by IEC/EN 60601-1-2. These limits are designed to provide a reasonable protection against electromagnetic interference in a typical medical installation.

Other devices may experience interference from even the low levels of electromagnetic emissions permitted by the above standards. To determine if the emissions from the XPO₂ are causing the interference, turn the XPO₂ Off. If the interference with the other device(s) stops, then the XPO₂ is causing the interference. In such rare cases, interference may be reduced or corrected by one of the following measures:

- Reposition, relocate, or increase the separation between the equipment.
- Connect the equipment into an outlet on a circuit different from that to which the other device(s) is connected.

SECTION 2—COMPONENT REPLACEMENT

CAUTION

Ensure not to damage ribbon cable when removing or installing front cover.
DO NOT use Methyl Ethyl Ketone (MEK). This will damage the plastic.

Replacing the Gross Particle Filter or Filter Cover

NOTE: For this procedure, refer to FIGURE 2.1.

NOTE: The gross particle filter should be replaced as needed.

1. Lift filter cover slightly and pull down to remove tabs from the grooves.
2. Lift out the filter from the filter cover.
3. Use a vacuum cleaner or wash with a mild liquid dish detergent (such as Dawn™) and water. Rinse thoroughly.
4. Thoroughly dry the filter and inspect for fraying, crumbling, tears and holes.
5. Replace filter cover and/or filter.
6. Reinstall the filter cover by placing the tabs in the slots and engaging the magnet.

NOTE: Use only Invacare gross particle filter.

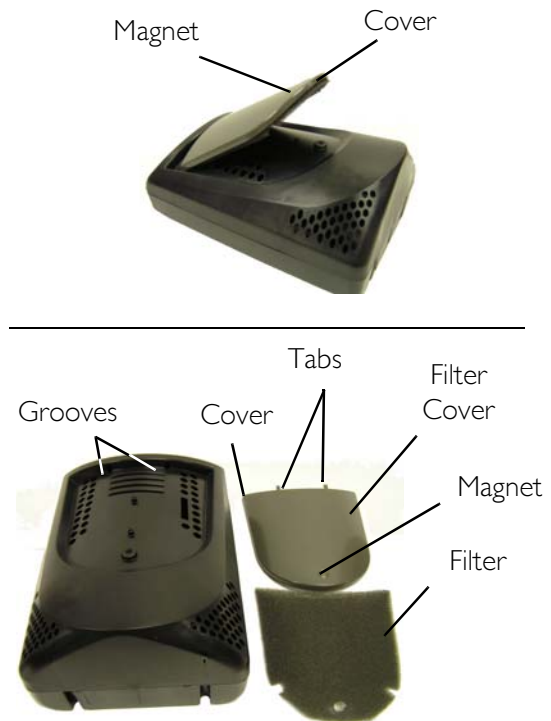


FIGURE 2.1 Replacing the Gross Particle Filter or Filter Cover

Accessing XPO₂

⚠ WARNING

When accessing the XPO₂ remember that battery power is still being applied to the internal (PCB) printed circuit board. Care **MUST** be taken to minimize contact with the PCB. **DO NOT** use any kind of tool (screwdriver, pliers, etc.) when working on the internal structure, otherwise, injury and/or damage may occur. Battery power remains on the PCB as long as the battery connection is made to the PCB.

NOTE: For this procedure, refer to FIGURE 2.2 and FIGURE 2.3 on page 10.

1. Remove label from the top of the XPO₂ (FIGURE 2.2).

NOTE: This label adheres to the front and rear sections of the XPO₂. This label MUST be removed to separate the two sections.



FIGURE 2.2 Remove/Install label

2. Position the XPO₂ so that the back panel label is facing up (Detail “A” in FIGURE 2.3).
3. Remove the four mounting screws from the back of the XPO₂ using a T15 Torx[®] screwdriver (Detail “A” in FIGURE 2.3).

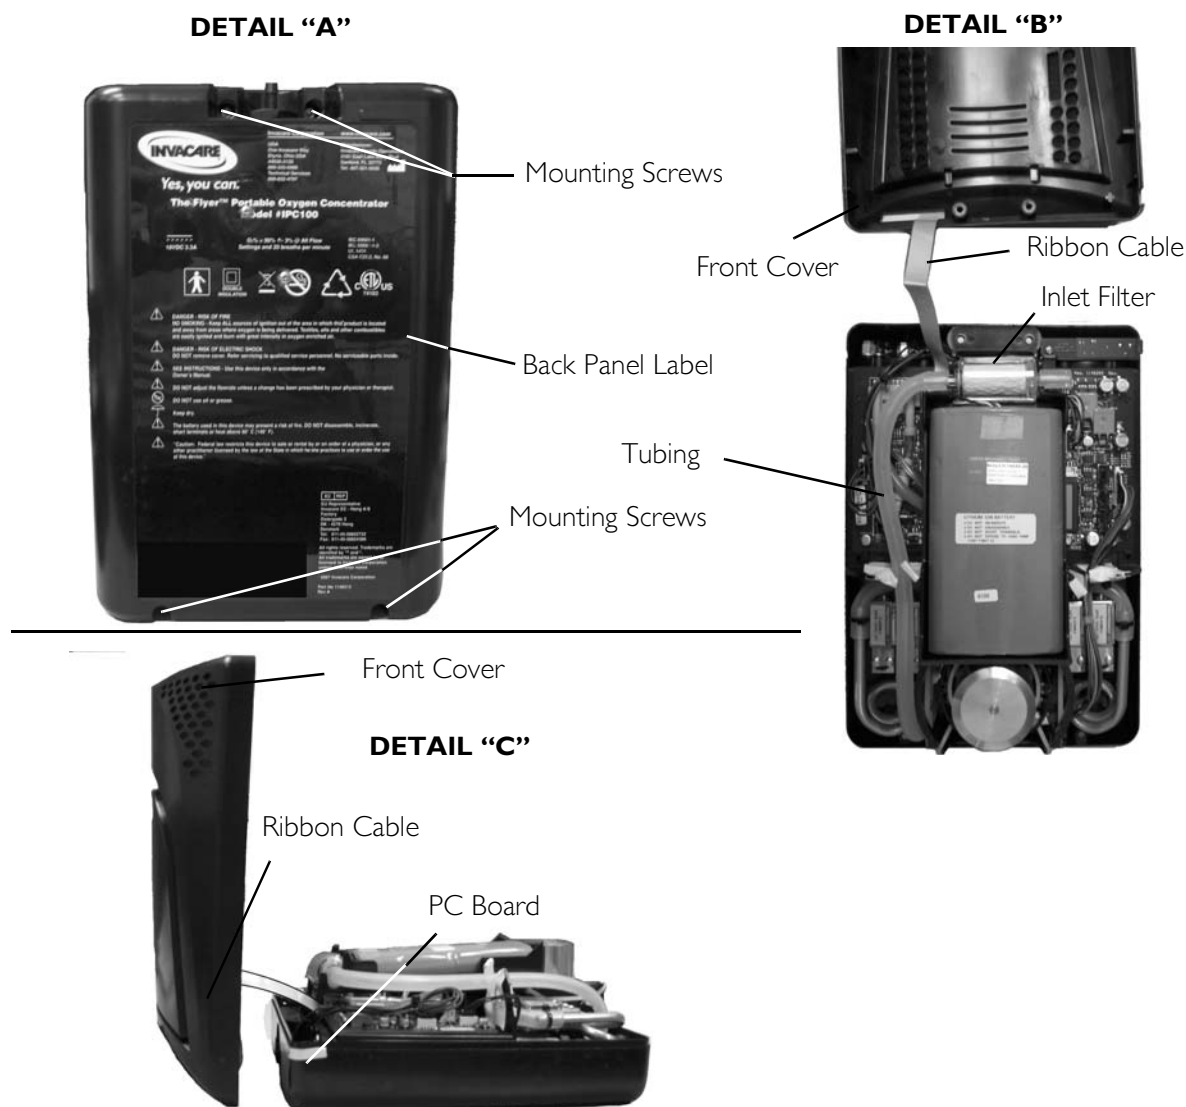


FIGURE 2.3 Removing the Front Cover

4. While holding the unit together rotate the XPO₂ and position it so that the back panel label is facing down.

NOTE: The ribbon cable is connected to the front cover and the pc board. Only open the XPO₂ as shown in Details “B” and “C”.

5. Slowly, open the front cover ensuring not to damage the ribbon cable (Detail “B” and Detail “C” in FIGURE 2.3).

Replacing the Inlet Filter

NOTE: For this procedure, refer to FIGURE 2.4 and FIGURE 2.2 on page 10.

NOTE: The inlet filter should be replaced as needed.

1. Perform the steps in [Accessing XPO₂](#) on page 9.
2. Remove the inlet filter from the holder (Detail “A”).
3. Disconnect the inlet filter with ⁵/₈-inch tubing attached from the 1 1/2-inch long tubing (Detail “B”).

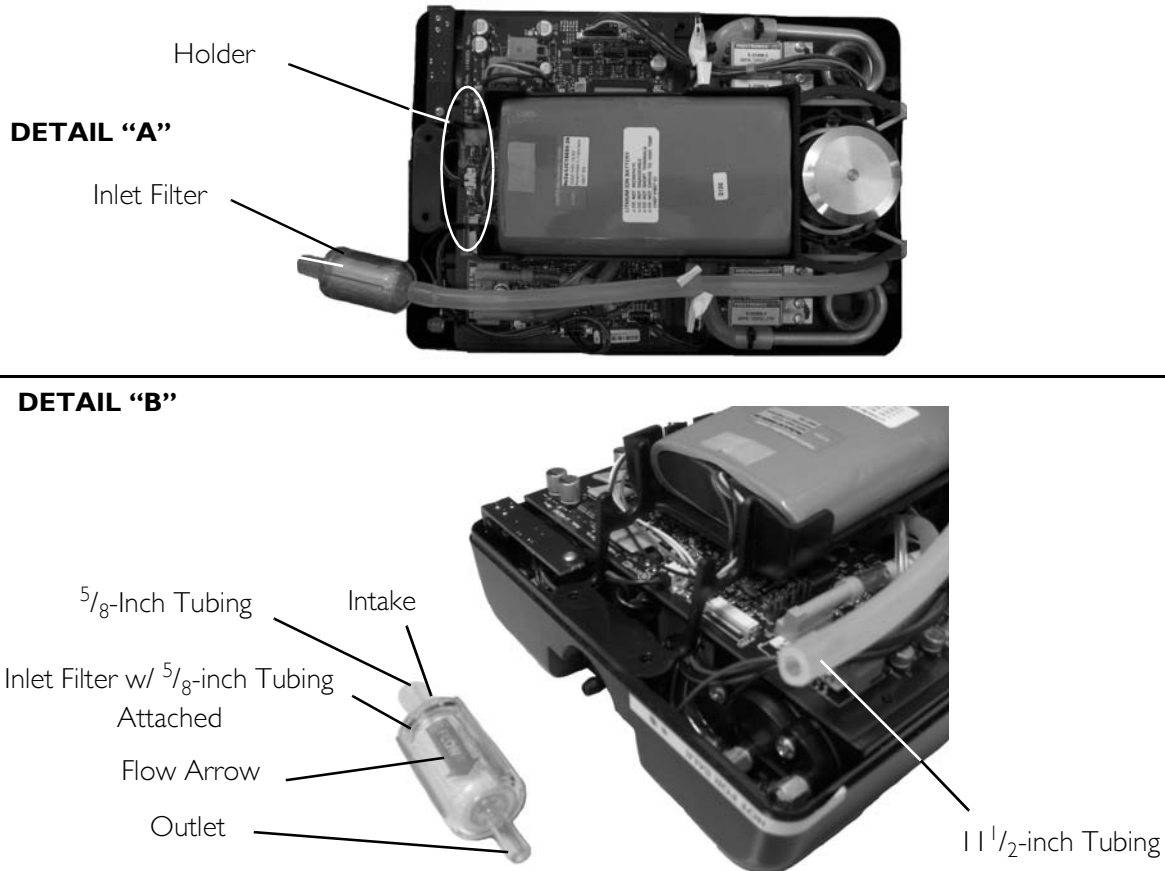


FIGURE 2.4 Replacing the Inlet Filter

4. Transfer the $\frac{5}{8}$ -inch tubing to the intake of the new filter.

NOTE: The flow arrow points away from the intake.

5. Connect the 11½-inch tubing to the outlet of the inlet filter (Detail “A” of FIGURE 2.4).
6. Position and orient the new filter in the holder (Detail “B” of FIGURE 2.3).
7. Re-assemble the XPO₂. Refer to Re-assembling the XPO₂ on page 13.

Replacing the Battery

CAUTION

Before handling the P.C. board, ensure you are properly grounded to prevent static damage to the components of the board. A static cuff **MUST** be worn and properly grounded using an alligator clip. Electrical conduit or a water pipe is normally sufficient when a known good ground is unavailable. Care should be taken to ensure that the alligator clip contacts a bare metal surface.

NOTE: For this procedure, refer to FIGURE 2.5.

1. Perform the steps in Accessing XPO₂ on page 9.
2. Remove the inlet filter with tubing attached from the holder.
3. Disconnect the battery wiring harness from the PC board.
4. Remove the battery from the thermal pad and battery tray.

*NOTE: The thermal pad is between the battery and the bottom of the tray. It is a soft “dough-like” material that adheres to the tray. If thermal pad is damaged or pulled up during battery removal it **MUST** be replaced.*

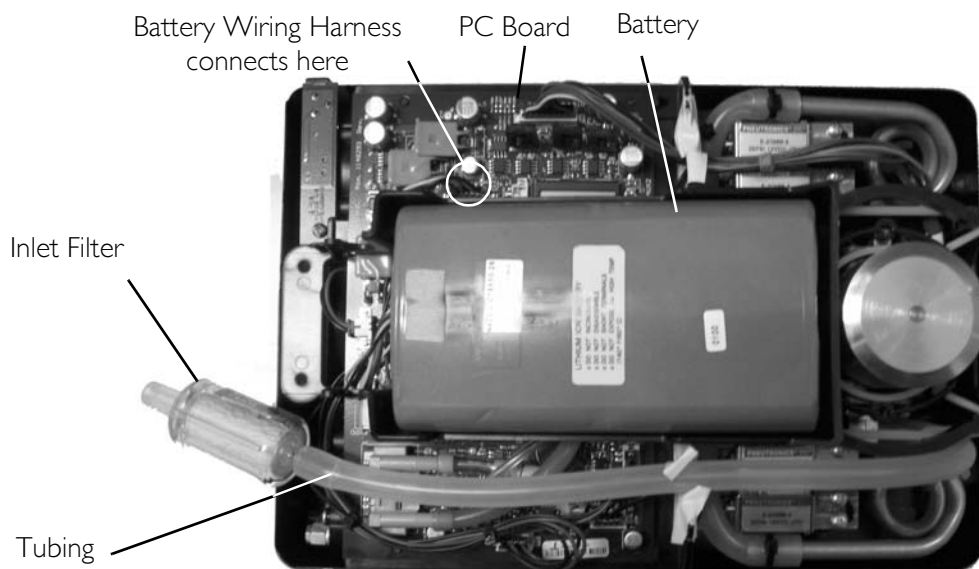


FIGURE 2.5 Replacing the Battery

NOTE: When installing new battery, ensure the battery is label side up.

5. Position new battery on thermal pad as shown.
6. Connect the battery wiring harness to the PC board.
7. Install inlet filter with tubing into holder.
8. Re-assemble the XPO₂. Refer to Re-assembling the XPO₂ on page 13.

Re-assembling the XPO₂

NOTE: For this procedure, refer to FIGURE 2.3 on page 10.

1. Carefully, re-install the front cover onto the XPO₂.
2. Turn the XPO₂ On to ensure proper operation.
3. Turn XPO₂ Off.
4. While holding the unit together, position the XPO₂ so that the back panel is facing up (Detail "A" in FIGURE 2.3).
5. Install four mounting screws and secure the two sections of the XPO₂ together (Detail "A" in FIGURE 2.3). Securely tighten.
6. Remove the glue residue by applying 91% isopropyl alcohol, and wiping with a clean cloth. Make sure the surface is dry and free of any residue. This will ensure a good seal for the new label.
7. Install replacement label on the top of the XPO₂ so that it adheres to both the front and rear sections.

Replacement Parts

NOTE: Refer to the parts catalog at www.invacare.com for component part number.

SECTION 3—CHECKING O₂ PURITY

NOTE: Although the XPO₂ offers pulse dose only, the oxygen purity can be checked with a hand held oxygen analyzer.

NOTE: Oxygen purity should be checked every 4,320 hours.

1. Turn the unit On.
2. Press the “+” button to increase the flow to setting 5.
3. Simultaneously press and hold the “+” and “battery gauge” buttons until the #5 BLUE indicator light blinks. This is your indication that the unit is now in auto-pulse mode.

NOTE: The unit will remain in auto-pulse mode until it is set to a lower flow setting or is turned off.

4. Connect a standard hand held oxygen analyzer to the outlet port.
5. Follow the directions provided by the analyzer manufacturer. Some analyzers will also measure flow and pressure, but only if connected to a continuous flow of oxygen (so these options are not usable on this pulse only unit).

NOTE: The purity reading may fluctuate slightly due to the pulse flow. It is recommended that you record a high and a low over a 60 second time period. The XPO₂ is functioning properly when the purity levels are above 87%, after the 5 minute warm-up period.

SECTION 4—ERROR CODES

The XPO₂ has dozens of alarms that are being monitored on a continuous basis. The alarms are grouped into four main categories:

- **Common Alarms:** These are alarms for which the patient, or the provider, can take action to eliminate the issue. These alarms, and the corrective steps, are fully explained within the Owner's Manual (OM).
- **Operating Alarms:** This alarm group centers on the sieve beds and the PSA process. These are alarms for which there is no corrective action available to either the patient or the provider. However, there are sub-codes that can be accessed to help the Invacare service and repair centers.
- **Compressor Alarms:** This alarm group centers on the compressor operation. These are alarms for which there is no corrective action available to either the patient or the provider. However, there are sub-codes that can be accessed to help the Invacare service and repair centers.
- **System Alarms:** This alarm group centers on internal software monitors. These are alarms for which there is no corrective action available to either the patient or the provider (*). However, there are sub-codes that can be accessed to help the Invacare service and repair centers.

To access the Sub-Alarm codes, the unit first has to be in an alarm condition with multiple flow level LEDs illuminated. While in this condition, the Plus (+) and Minus (-) flow setting buttons should be pushed and held. As long as both these buttons are being pushed, a different set of flow LEDs will illuminate. This alternate set of illuminated LEDs is the sub-alarm code. Once the Plus and Minus buttons are released, the original alarm code will return. Once the unit is turned off, the alarm codes displays will be reset. All the alarms should be reset and the unit turned back on to see if the unit can self-correct the problem. If the alarms persist, please contact your nearest Invacare repair center.

ERROR / ERROR CODE	ALARM (Illuminated flow LEDs)	SUB-ALARM (Illuminated flow LEDs)
Common Alarms		
Internal temperature of the unit is either too hot, or too cold, to allow compressor to start. See OM for instructions.	1, 2	None
While operating, the internal temperature of the unit becomes either too hot, or too cold, to allow operation to continue. See OM for instructions.	1, 3	None
The internal battery temperature is either too hot, or too cold, to allow operation on battery to continue. See OM for instructions.	1, 4	None
Control panel button was found to be continuously pressed upon power-up (a.k.a. stuck button). See OM for instructions.	1, 5	None
Operating Alarms		
Code: 3000	3, 4	None
Code: 3001	3, 4	1
Code: 3002	3, 4	2

SECTION 4—ERROR CODES

Compressor Alarms		
Code: 6000	4, 5	None
Code: 6001	4, 5	1
Code: 6002	4, 5	2
Code: 6003	4, 5	1,2

(*) Within the System Alarms there are a few alarms that *may* correct themselves simply by changing the internal battery.

ERROR/ ERROR CODE	ALARM (Illuminated flow LEDs)	SUB-ALARM (Illuminated flow LEDs)	COMMENTS
System Alarms			
Code: 7000	3, 4, 5	None	
Code: 7001	3, 4, 5	1	
Code: 7002	3, 4, 5	2	Replacement of the internal battery may eliminate this problem
Code: 7003	3, 4, 5	1,2	
Code: 7004	3, 4, 5	3	
Code: 7005	3, 4, 5	3,1	
Code: 7006	3, 4, 5	3,2	
Code: 7007	3, 4, 5	3,2,1	
Code: 7008	3, 4, 5	4	
Code: 7009	3, 4, 5	4,1	
Code: 700a	3, 4, 5	4,2	
Code: 700b	3, 4, 5	4,2,1	
Code: 700c	3, 4, 5	4,3	
Code: 700d	3, 4, 5	4,3,1	
Code: 700e	3, 4, 5	4,3,2	Replacement of the internal battery may eliminate this problem
Code: 700f	3, 4, 5	4,3,2,1	Replacement of the internal battery may eliminate this problem
Code: 7010	3, 4, 5	5	Replacement of the internal battery may eliminate this problem
Code: 7011	3, 4, 5	5,1	
Code: 7012	3, 4, 5	5,2	
Code: 7013	3, 4, 5	5,2,1	
Code: 7014	3, 4, 5	5,3	
Code: 7015	3, 4, 5	5,3,1	
Code: 7016	3, 4, 5	5,3,2	
Code: 7017	3, 4, 5	5,3,2,1	
Code: 7018	3, 4, 5	5,4	
Code: 7019	3, 4, 5	5,4,1	
Code: 701a	3, 4, 5	5,4,2	
Code: 701b	3, 4, 5	5,4,2,1	
Code: 701c	3, 4, 5	5,4,3	
Code: 701d	3, 4, 5	5,4,3,1	Replacement of the internal battery may eliminate this problem
Code: 701e	3, 4, 5	5,4,3,2	
Code: 701f	3, 4, 5	5,4,3,2,1	

NOTES

NOTES

LIMITED WARRANTY

For warranty information, please refer to the original owner's manual which came with this product, or contact Invacare for more information.



Yes, you can.

Invacare Corporation www.invacare.com

USA
One Invacare Way
Elyria, Ohio USA
44036-2125
800-333-6900

Canada
570 Matheson Blvd E Unit 8
Mississauga Ontario
L4Z 4G4 Canada
800-668-5324

All rights reserved. Trademarks are identified by [™] and [®]. All trademarks are owned by or licensed to Invacare Corporation unless otherwise noted. Torx is a registered trademark of Textron, Inc. Dawn is a trademark of The Proctor and Gamble Company.
© 2008 Invacare Corporation

Part No 1150748

Rev A - 4/08

Free Manuals Download Website

<http://myh66.com>

<http://usermanuals.us>

<http://www.somanuals.com>

<http://www.4manuals.cc>

<http://www.manual-lib.com>

<http://www.404manual.com>

<http://www.luxmanual.com>

<http://aubethermostatmanual.com>

Golf course search by state

<http://golfingnear.com>

Email search by domain

<http://emailbydomain.com>

Auto manuals search

<http://auto.somanuals.com>

TV manuals search

<http://tv.somanuals.com>